


XX XX
ID: XX Page: Acq Test Date: Jun. 04, 2024 DOB: Age: (DOB empty) Report: Jun. 04, 2024
Acquisition Page



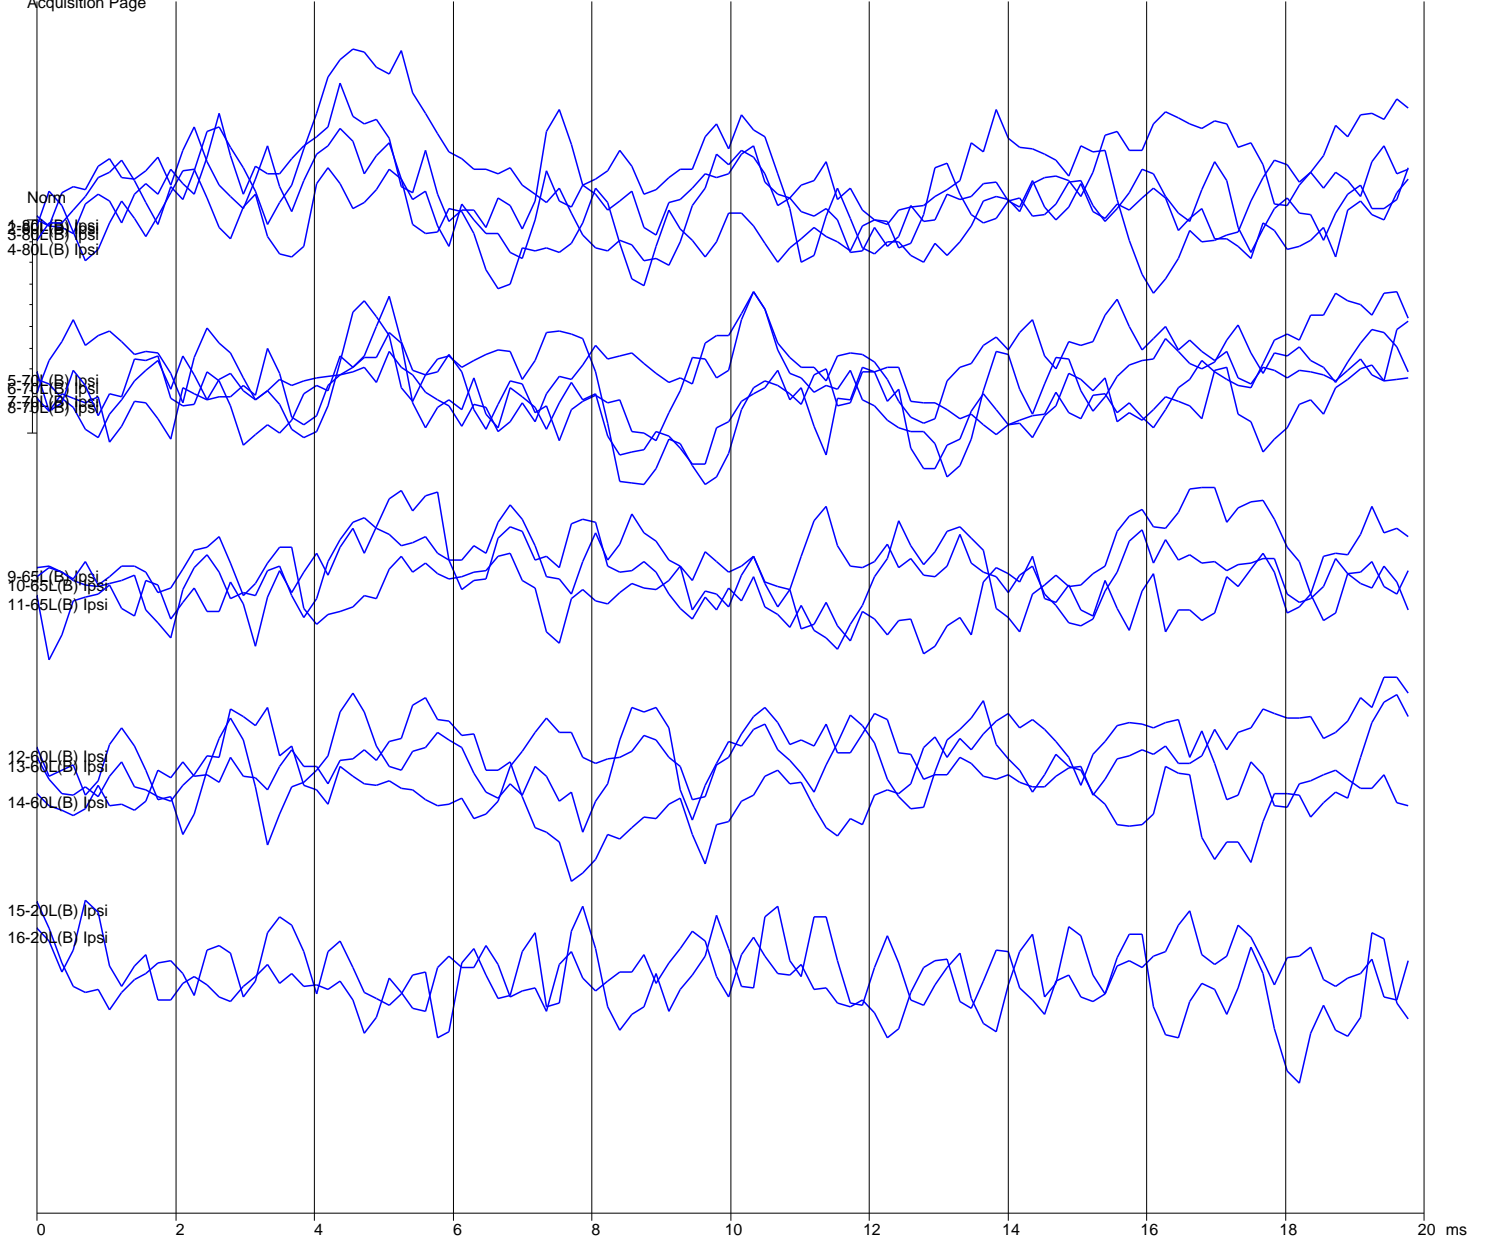

6860 SW 81st Street Miami, Florida 33143
 305-668-6102 • 1-800-IHSYSTEMS • www.ihsys.com

XX XX
 ID: XX Page: Acq Test Date: Jun. 04, 2024 DOB: Age: (DOB empty) Report: Jun. 04, 2024
 Acquisition Page

Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	LXLA80B.3	80SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.29	0.05 2.221	100	100-1500Hz
2	LXLA80B.1	80SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.43	0.07 2.085	100	100-1500Hz
3	LXLA80B.2	80SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.41	0.06 2.171	100	100-1500Hz
4	LXLA80B.4	80SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.31	0.07 2.645	100	100-1500Hz
5	LXLA70B.3	70SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.28	0.10 0.776	100	100-1500Hz
6	LXLA70B.2	70SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.33	0.21 0.739	100	100-1500Hz
7	LXLA70B.4	70SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.32	0.07 0.938	100	100-1500Hz
8	LXLA70B.1	70SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.30	0.13 0.725	100	100-1500Hz
9	LXLA65B.3	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.33	0.17 0.464	100	100-1500Hz
10	LXLA65B.2	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.36	0.17 0.432	100	100-1500Hz
11	LXLA65B.1	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.29	0.18 0.425	100	100-1500Hz
12	LXLA60B.3	60SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.27	0.31 0.263	100	100-1500Hz
13	LXLA60B.2	60SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.34	0.25 0.352	100	100-1500Hz
14	LXLA60B.1	60SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.34	0.26 0.629	100	100-1500Hz
15	LXLA20B.2	20SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.21	0.27 0.231	100	100-1500Hz
16	LXLA20B.1	20SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.28	0.27 0.200	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms *-indicates different region used

Num	Int	Ear	Peaks: Latency(ms) Amp(uV) (AR=Amp Ratio)
1	80	L	
2	80	L	
3	80	L	
4	80	L	
5	70	L	
6	70	L	
7	70	L	
8	70	L	
9	65	L	
10	65	L	
11	65	L	
12	60	L	
13	60	L	
14	60	L	
15	20	L	
16	20	L	