


XX XX
 ID: XX Page: Acq Test Date: May, 28, 2024 DOB: Age: (DOB empty) Report: May, 28, 2024
 Acquisition Page

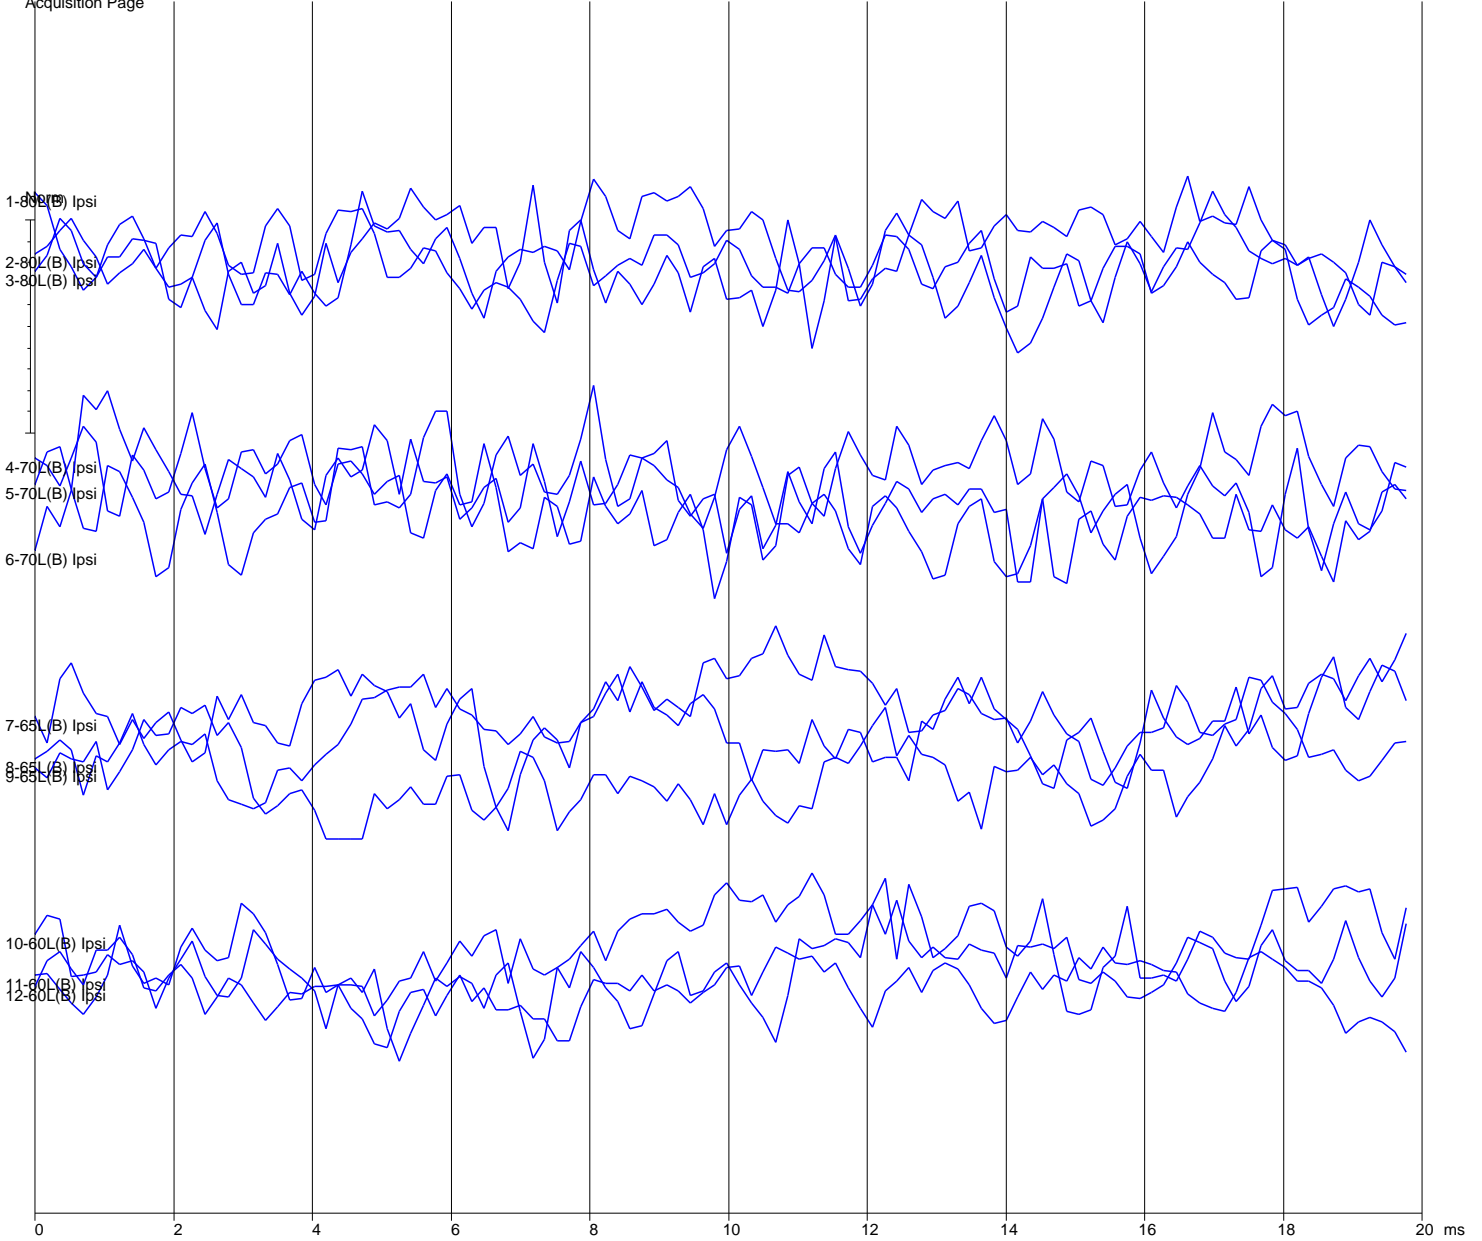

Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	DXLA80B.1	80SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.30	0.03 2.488	100	100-1500Hz
2	DXLA80B.2	80SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.21	0.03 2.394	100	100-1500Hz
3	DXLA80B.3	80SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.35	0.05 2.327	100	100-1500Hz
4	DXLA70B.3	70SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.21	0.08 0.794	100	100-1500Hz
5	DXLA70B.1	70SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.27	0.11 0.807	100	100-1500Hz
6	DXLA70B.2	70SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.20	0.07 0.761	100	100-1500Hz
7	DXLA65B.2	65SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.21	0.11 0.719	100	100-1500Hz
8	DXLA65B.1	65SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.23	0.12 0.513	100	100-1500Hz
9	DXLA65B.3	65SPL	L	Bone	500Hz(1)	560/1	11.4	Altr	0.18	0.06 0.726	100	100-1500Hz
10	DXLA60B.2	60SPL	L	Bone	500Hz(1)	560/0	11.4	Altr	0.23	0.18 0.335	100	100-1500Hz
11	DXLA60B.1	60SPL	L	Bone	500Hz(1)	560/0	11.4	Altr	0.24	0.12 0.467	100	100-1500Hz
12	DXLA60B.3	60SPL	L	Bone	500Hz(1)	560/0	11.4	Altr	0.28	0.12 0.439	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms *-indicates different region used

Num	Int	Ear	Peaks: Latency(ms) Amp(uV) (AR=Amp Ratio)
1	80	L	
2	80	L	
3	80	L	
4	70	L	
5	70	L	
6	70	L	
7	65	L	
8	65	L	
9	65	L	
10	60	L	
11	60	L	
12	60	L	