


XX XX  
ID: XX Page: Acq Test Date: May. 28, 2024 DOB: Age: (DOB empty) Report: May. 28, 2024  
Acquisition Page



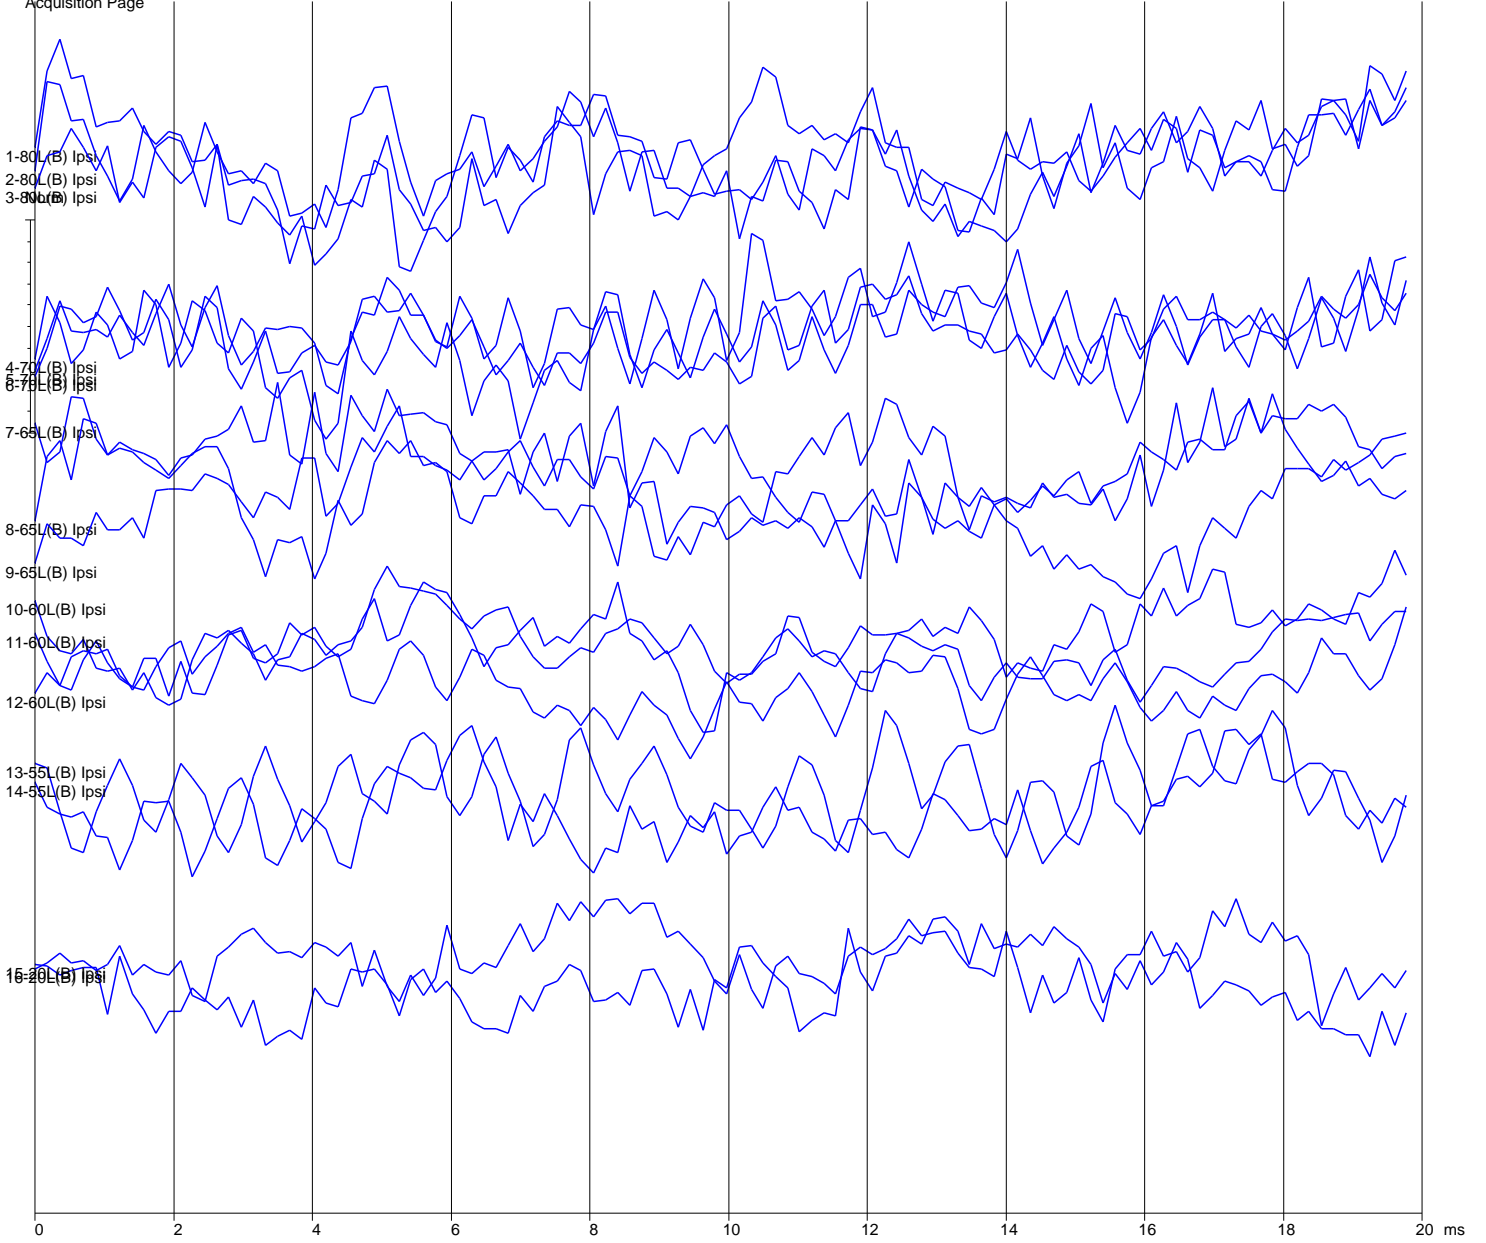

6860 SW 81st Street Miami, Florida 33143  
 305-668-6102 • 1-800-IHSYSTEMS • www.ihsys.com

XX XX  
 ID: XX Page: Acq Test Date: May. 28, 2024 DOB: Age: (DOB empty) Report: May. 28, 2024  
 Acquisition Page

Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	DXLA80B.3	80SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.40	0.03 7.582	100	100-1500Hz
2	DXLA80B.2	80SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.40	0.02 7.829	100	100-1500Hz
3	DXLA80B.1	80SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.36	0.02 7.196	100	100-1500Hz
4	DXLA70B.1	70SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.30	0.04 2.359	100	100-1500Hz
5	DXLA70B.3	70SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.37	0.04 2.513	100	100-1500Hz
6	DXLA70B.2	70SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.40	0.05 2.344	100	100-1500Hz
7	DXLA65B.1	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.40	0.08 1.533	100	100-1500Hz
8	DXLA65B.2	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.50	0.10 1.476	100	100-1500Hz
9	DXLA65B.3	65SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.44	0.04 2.026	100	100-1500Hz
10	DXLA60B.1	60SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.29	0.08 0.850	100	100-1500Hz
11	DXLA60B.3	60SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.29	0.08 0.832	100	100-1500Hz
12	DXLA60B.2	60SPL	L	Bone	6000Hz(1)	560/0	11.4	Altr	0.25	0.06 0.842	100	100-1500Hz
13	DXLA55B.1	55SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.63	0.25 0.786	100	100-1500Hz
14	DXLA55B.2	55SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.23	0.18 0.472	100	100-1500Hz
15	DXLA20B.1	20SPL	L	Bone	6000Hz(1)	560/1	11.4	Altr	0.21	0.06 0.710	100	100-1500Hz
16	DXLA20B.2	20SPL	L	Bone	6000Hz(1)	54/1	11.4	Altr	0.83	0.08 3.142	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms \*-indicates different region used

Num	Int	Ear	Peaks: Latency(ms)   Amp(uV) (AR=Amp Ratio)
1	80	L	
2	80	L	
3	80	L	
4	70	L	
5	70	L	
6	70	L	
7	65	L	
8	65	L	
9	65	L	
10	60	L	
11	60	L	
12	60	L	
13	55	L	
14	55	L	
15	20	L	
16	20	L	