


XX XX  
ID: XX Page: Acq Test Date: Jun. 03, 2024 DOB: Age: (DOB empty) Report: Jun. 04, 2024  
Acquisition Page



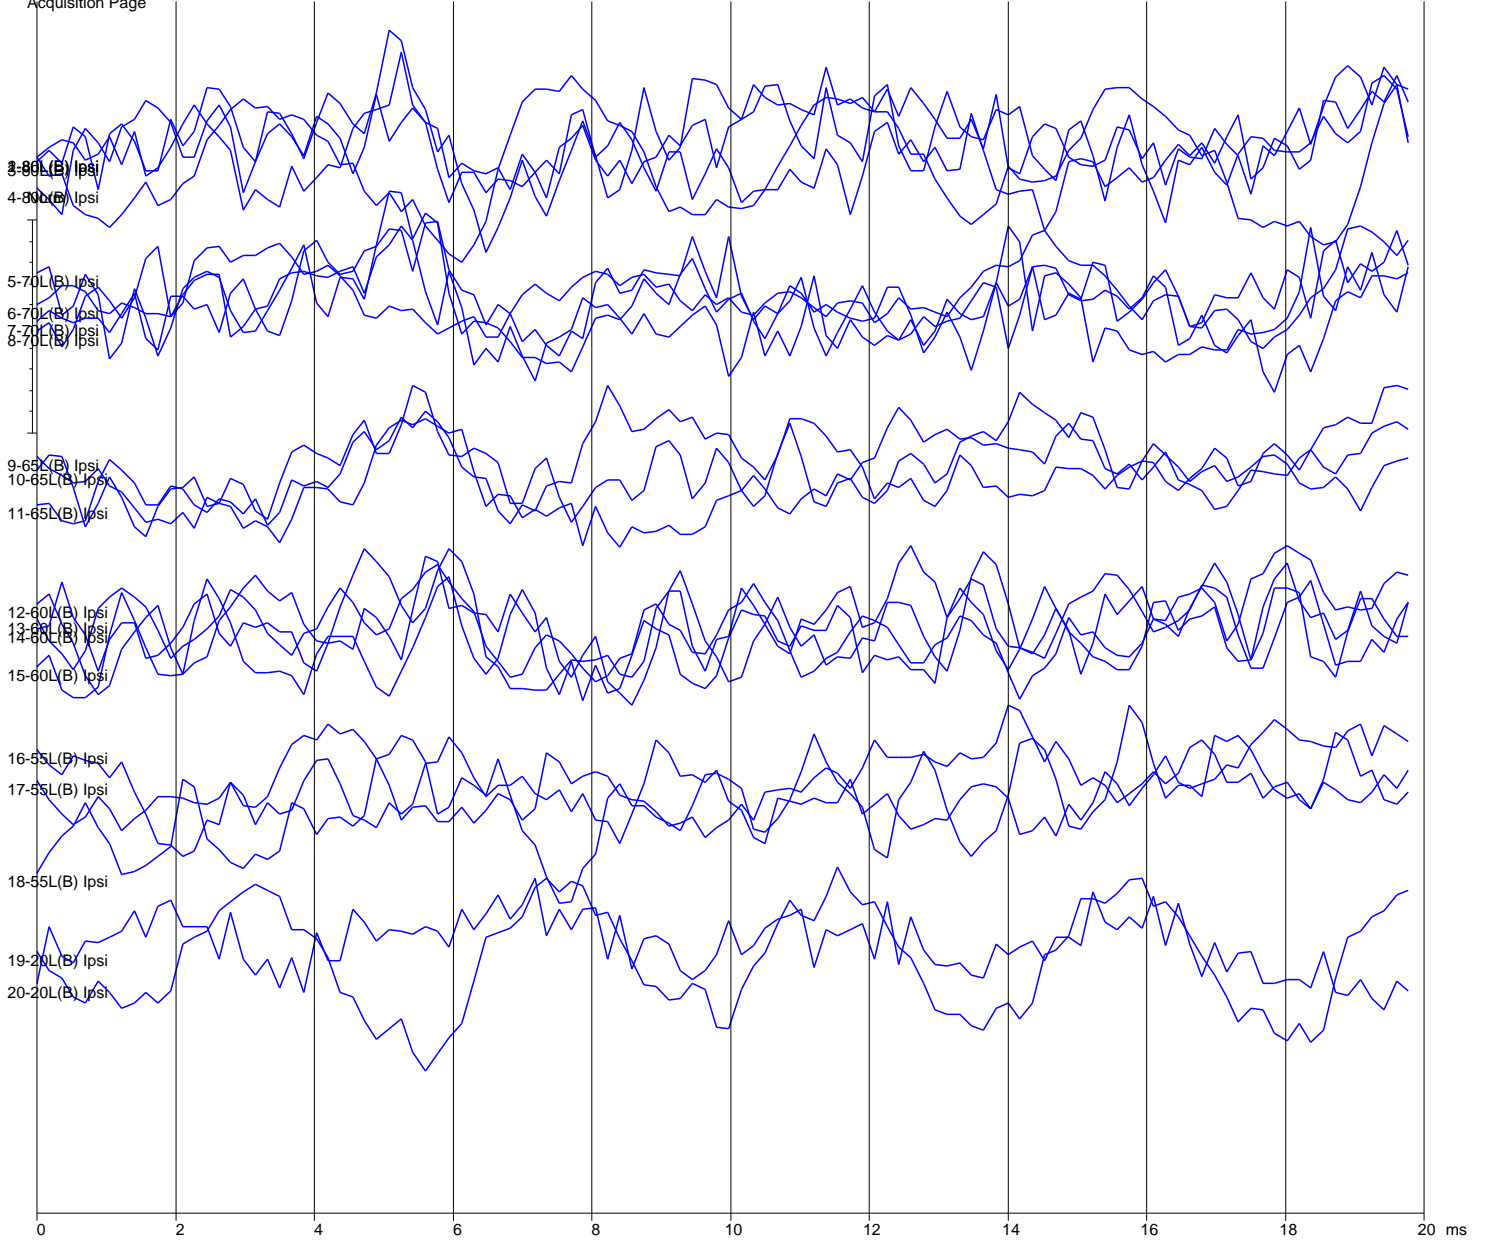

6860 SW 81st Street Miami, Florida 33143  
 305-668-6102 • 1-800-IHSYSTEMS • www.ihsys.com

XX XX  
 ID: XX Page: Acq Test Date: Jun. 03, 2024 DOB: Age: (DOB empty) Report: Jun. 04, 2024  
 Acquisition Page

Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	BXLA80B.2	80SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.43	0.02 7.111	100	100-1500Hz
2	BXLA80B.5	80SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	1.17	0.07 8.845	100	100-1500Hz
3	BXLA80B.3	80SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.43	0.02 6.220	100	100-1500Hz
4	BXLA80B.1	80SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.47	0.03 6.764	100	100-1500Hz
5	BXLA70B.2	70SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.35	0.07 2.298	100	100-1500Hz
6	BXLA70B.4	70SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.77	0.06 2.640	100	100-1500Hz
7	BXLA70B.1	70SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.38	0.06 2.156	100	100-1500Hz
8	BXLA70B.3	70SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.39	0.06 2.470	100	100-1500Hz
9	BXLA65B.2	65SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.32	0.09 1.387	100	100-1500Hz
10	BXLA65B.1	65SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.43	0.10 1.265	100	100-1500Hz
11	BXLA65B.3	65SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.36	0.09 1.272	100	100-1500Hz
12	BXLA60B.2	60SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.42	0.25 0.717	100	100-1500Hz
13	BXLA60B.3	60SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.42	0.19 0.672	100	100-1500Hz
14	BXLA60B.4	60SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.30	0.14 0.725	100	100-1500Hz
15	BXLA60B.1	60SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.49	0.13 1.185	100	100-1500Hz
16	BXLA55B.2	55SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.31	0.07 1.055	100	100-1500Hz
17	BXLA55B.1	55SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.37	0.13 0.829	100	100-1500Hz
18	BXLA55B.3	55SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.34	0.27 0.517	100	100-1500Hz
19	BXLA20B.1	20SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	1.15	0.15 4.128	100	100-1500Hz
20	BXLA20B.2	20SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.39	0.22 0.400	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms \*-indicates different region used

Num	Int	Ear	Peaks: Latency(ms)   Amp(uV) (AR=Amp Ratio)
1	80	L	
2	80	L	
3	80	L	
4	80	L	
5	70	L	
6	70	L	
7	70	L	
8	70	L	
9	65	L	
10	65	L	
11	65	L	
12	60	L	
13	60	L	
14	60	L	
15	60	L	
16	55	L	
17	55	L	
18	55	L	
19	20	L	
20	20	L	

1.00uV



Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	BXLA50B.1	50SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.46	0.39 0.337	100	100-1500Hz
2	BXLA50B.3	50SPL	L	Bone	8000Hz(1)	560/0	11.4	Altr	0.39	0.14 0.740	100	100-1500Hz
3	BXLA50B.2	50SPL	L	Bone	8000Hz(1)	560/1	11.4	Altr	0.32	0.11 0.667	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms \*-indicates different region used

Num	Int	Ear	Peaks: Latency(ms)   Amp(uV) (AR=Amp Ratio)
1	50	L	
2	50	L	
3	50	L	