


XX XX
 ID: XX Page: Acq Test Date: May. 28, 2024 DOB: Age: (DOB empty) Report: May. 28, 2024
 Acquisition Page

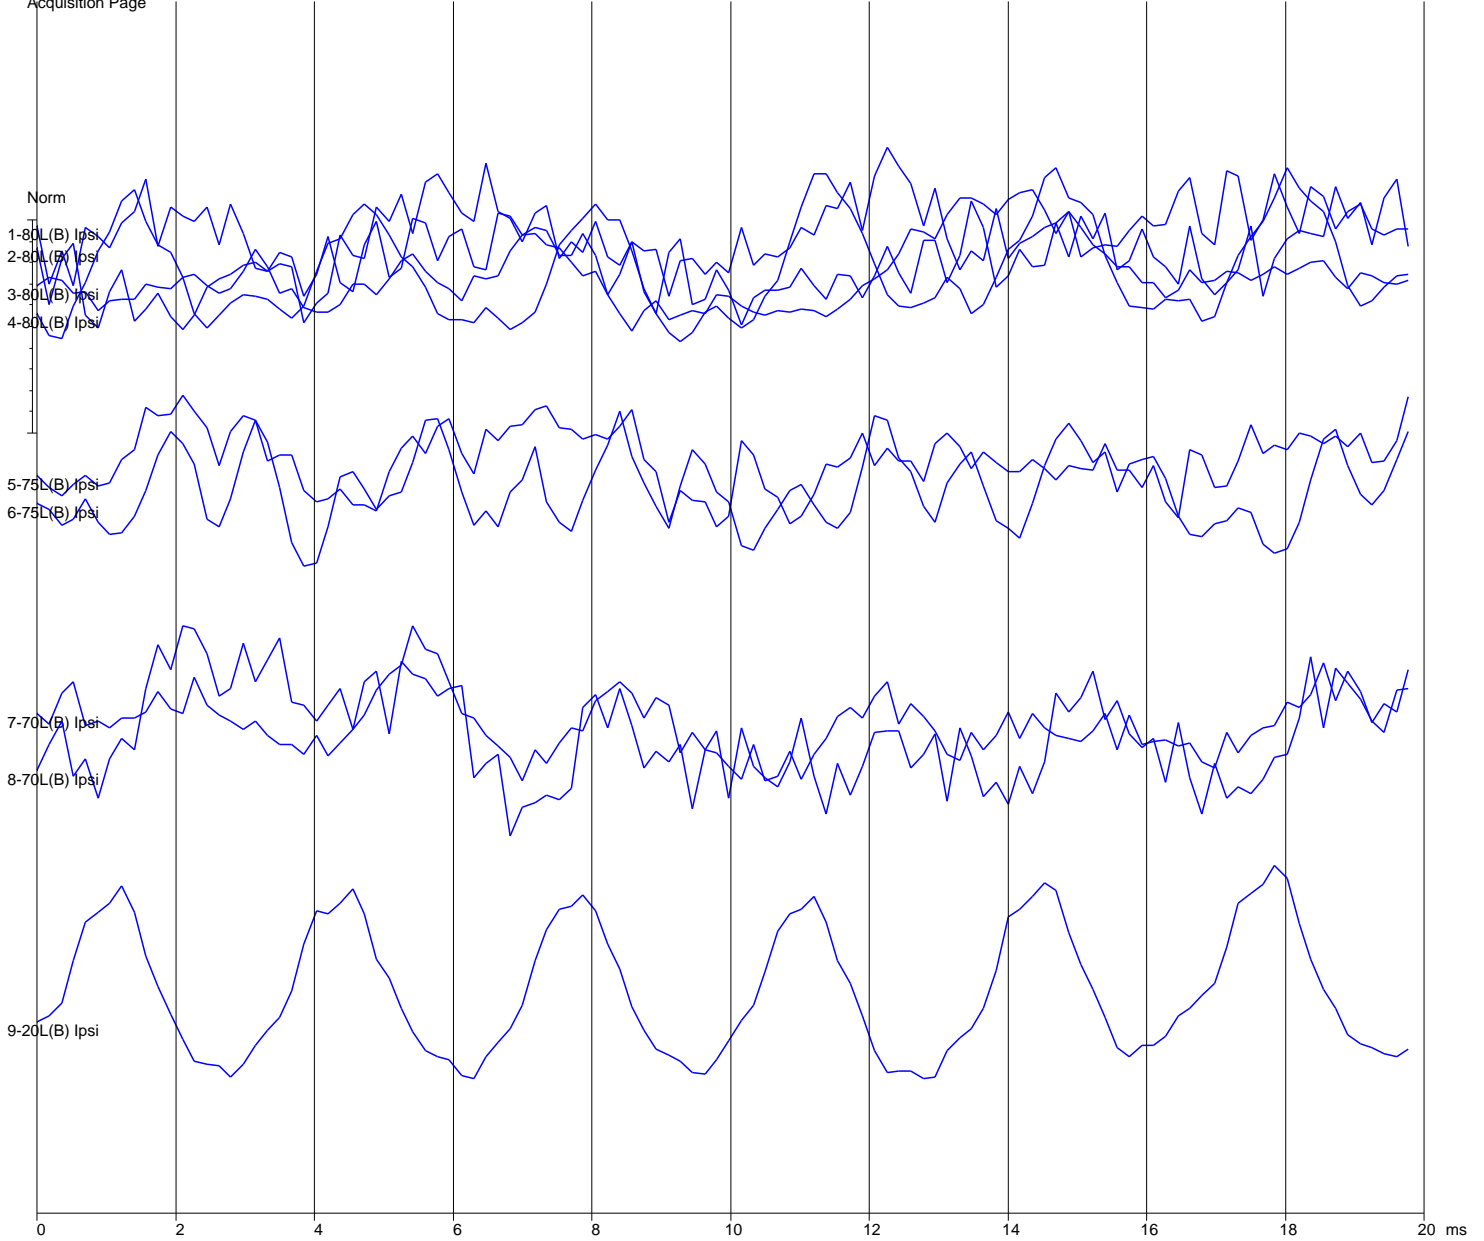

Num	Filename	Int	Ear	Stim.	Type	Swps/Art	Rate	Mode	PP Amp	SNR RN	Gain	Filters
1	DCLA80B.3	80SPL	L	Bone	Click	560/1	11.1	Altr	0.30	0.44 0.232	100	100-1500Hz
2	DCLA80B.1	80SPL	L	Bone	Click	560/1	11.4	Altr	0.35	0.34 0.252	100	100-1500Hz
3	DCLA80B.2	80SPL	L	Bone	Click	560/1	17.1	Altr	0.37	0.07 1.215	100	100-1500Hz
4	DCLA80B.4	80SPL	L	Bone	Click	560/1	11.1	Altr	0.71	2.26 0.124	100	100-1500Hz
5	DCLA75B.2	75SPL	L	Bone	Click	560/1	11.1	Altr	0.29	0.17 0.515	100	100-1500Hz
6	DCLA75B.1	75SPL	L	Bone	Click	560/0	11.1	Altr	0.40	0.66 0.218	100	100-1500Hz
7	DCLA70B.1	70SPL	L	Bone	Click	560/0	11.1	Altr	0.41	0.80 0.182	100	100-1500Hz
8	DCLA70B.2	70SPL	L	Bone	Click	560/1	11.1	Altr	0.26	0.29 0.409	100	100-1500Hz
9	DCLA20B.1	20SPL	L	Bone	Click	560/1	11.1	Altr	0.80	4.54 0.103	100	100-1500Hz

System SNR & RN Region: 4.00 - 9.00 ms * -indicates different region used

Num	Int	Ear	Peaks: Latency(ms) Amp(uV) (AR=Amp Ratio)
1	80	L	
2	80	L	
3	80	L	
4	80	L	
5	75	L	
6	75	L	
7	70	L	
8	70	L	
9	20	L	